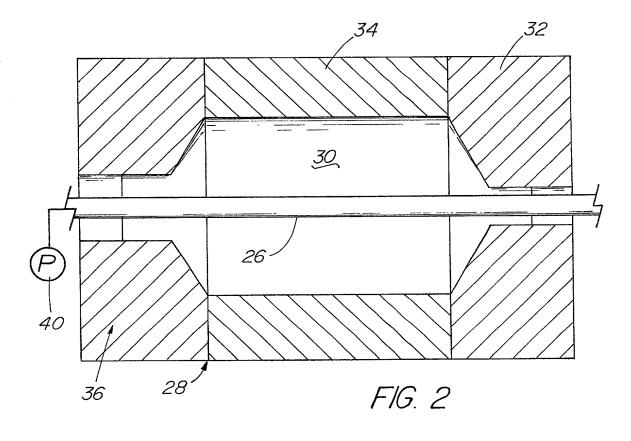
16

-10



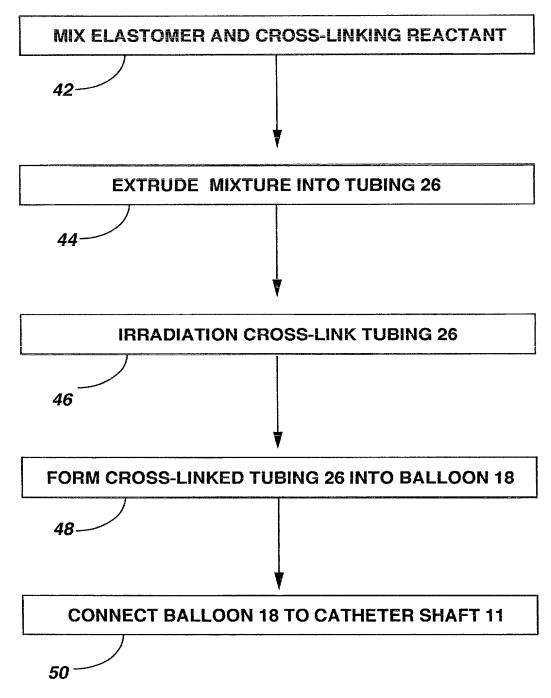
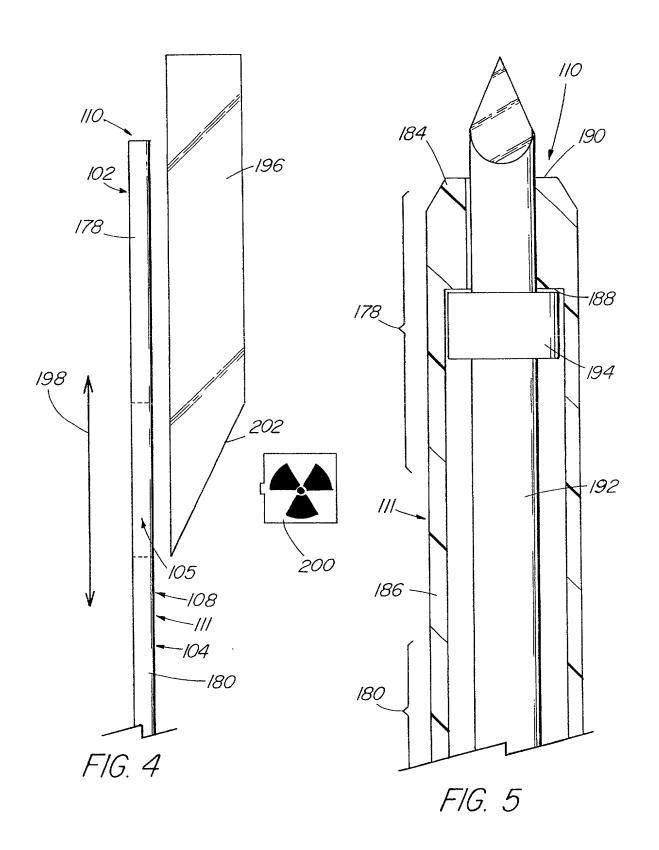
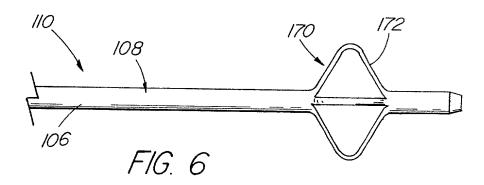


FIG. 3





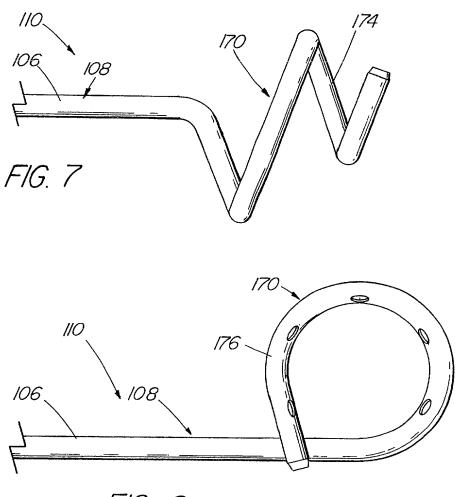


FIG. 8

In Re: Boatman et al.

Medical Device Including Unitary, Continuous
Portion of Varying Durometer

PA-5259-RFB

